

This Page Is Inserted by IFW Operations  
and is not a part of the Official Record

## **BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning documents *will not* correct images,  
please do not report the images to the  
Image Problem Mailbox.**

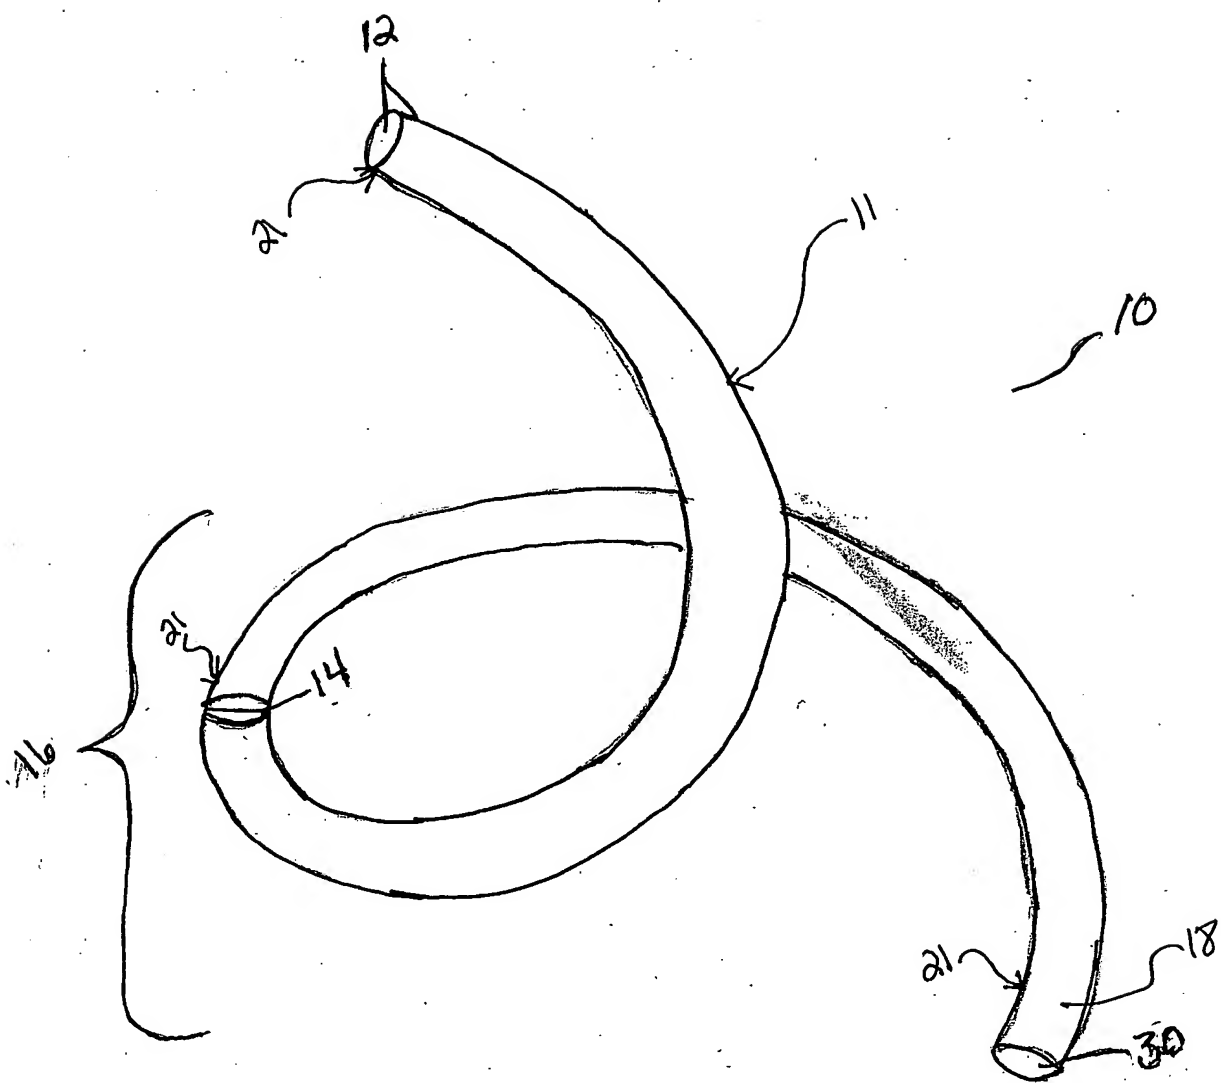


Fig. 1



FIG. 4


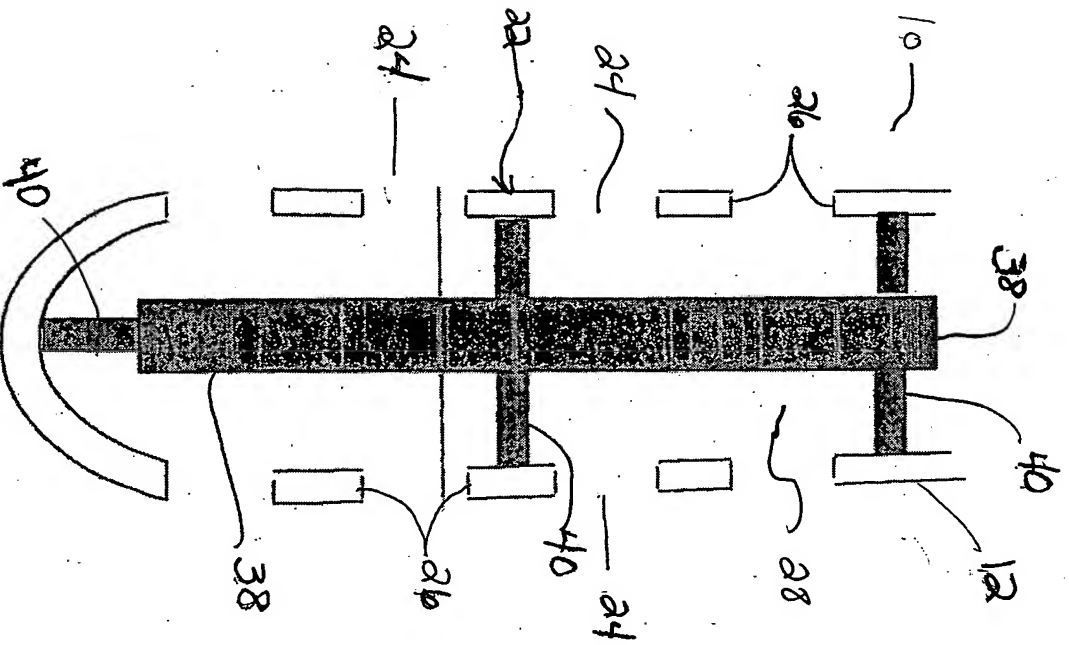


FIG. 5

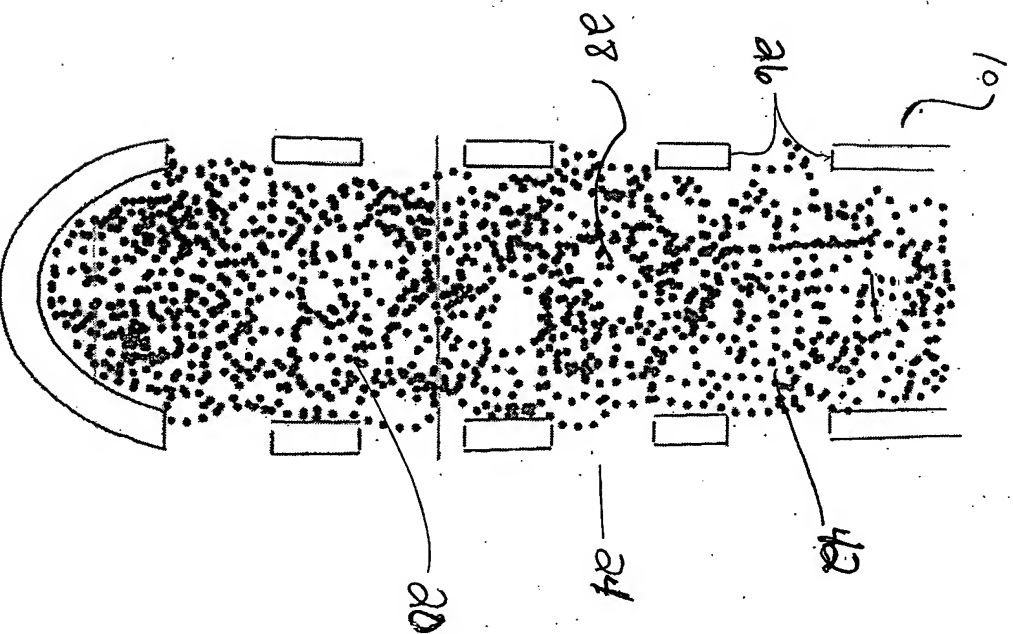

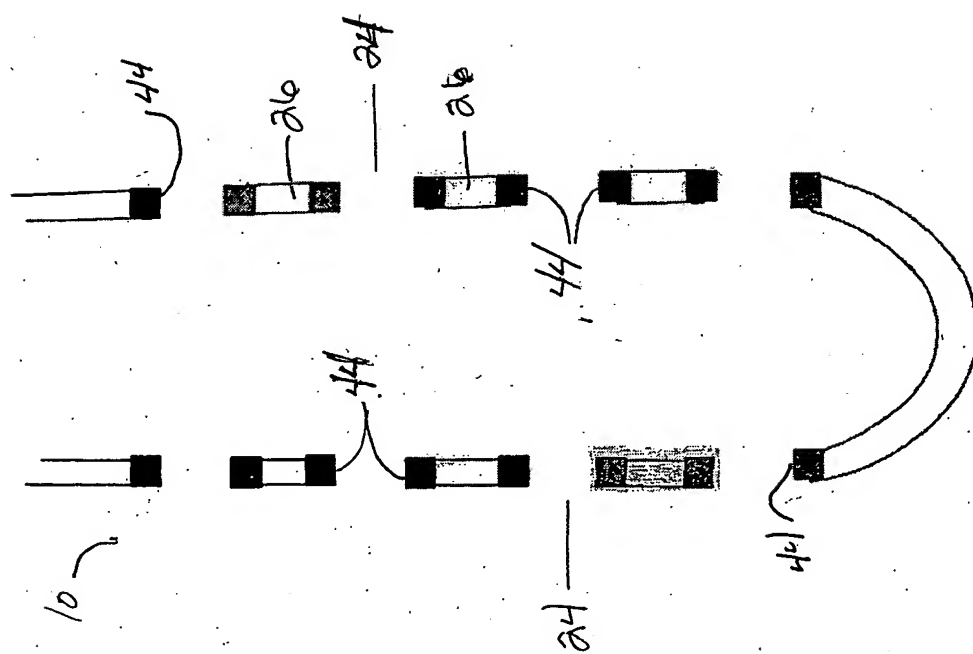
6  
b  
LI

Fig. 7



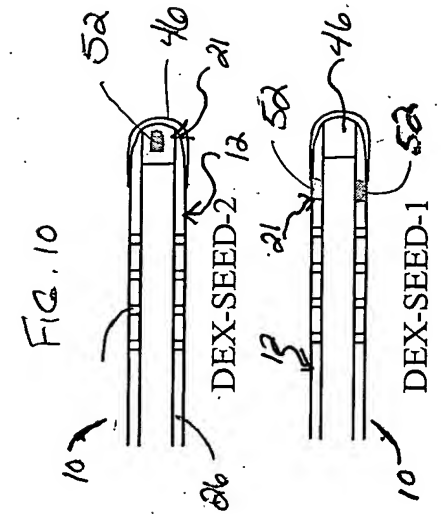
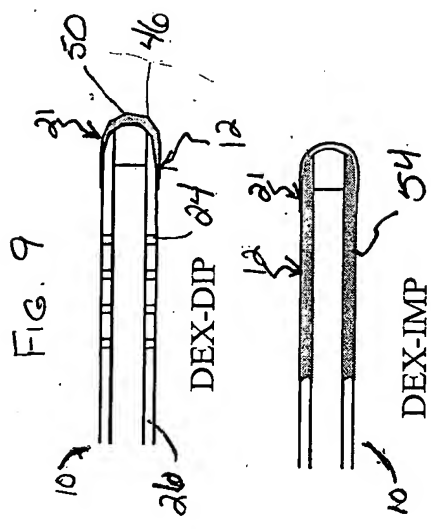
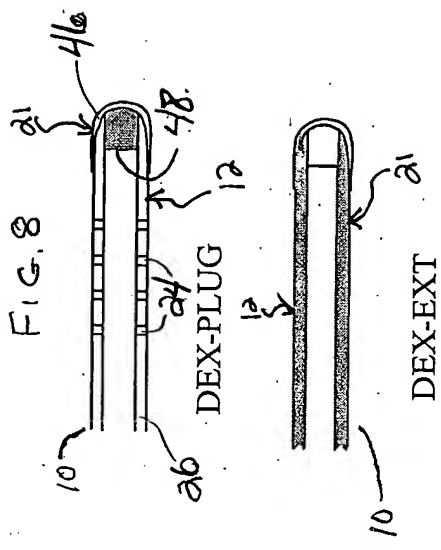


FIG. 13

FIG. 12

FIG. 11

FIG. 14

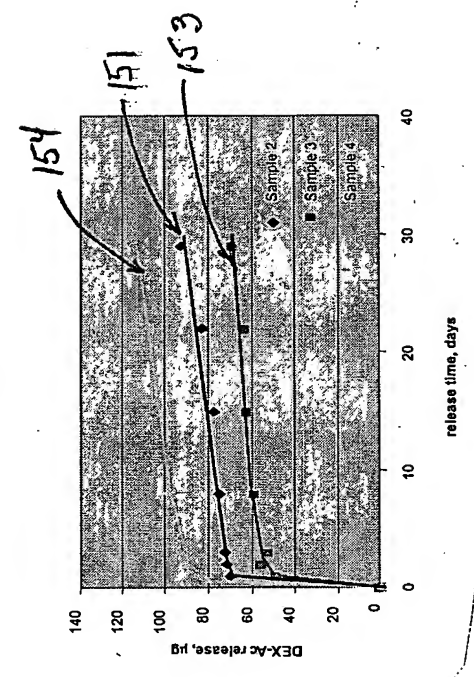


FIG. 15

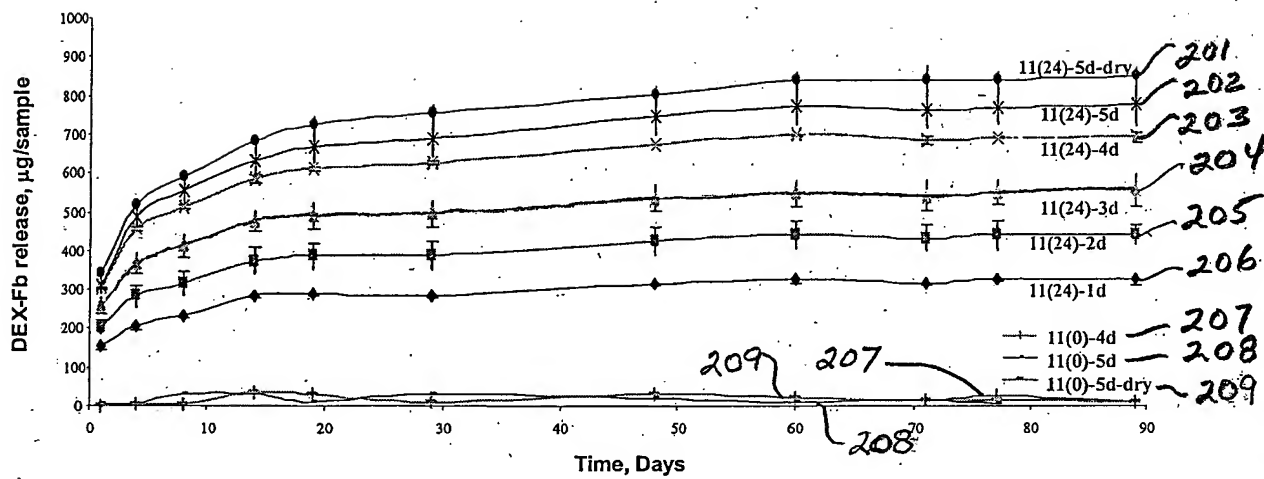


FIG. 16

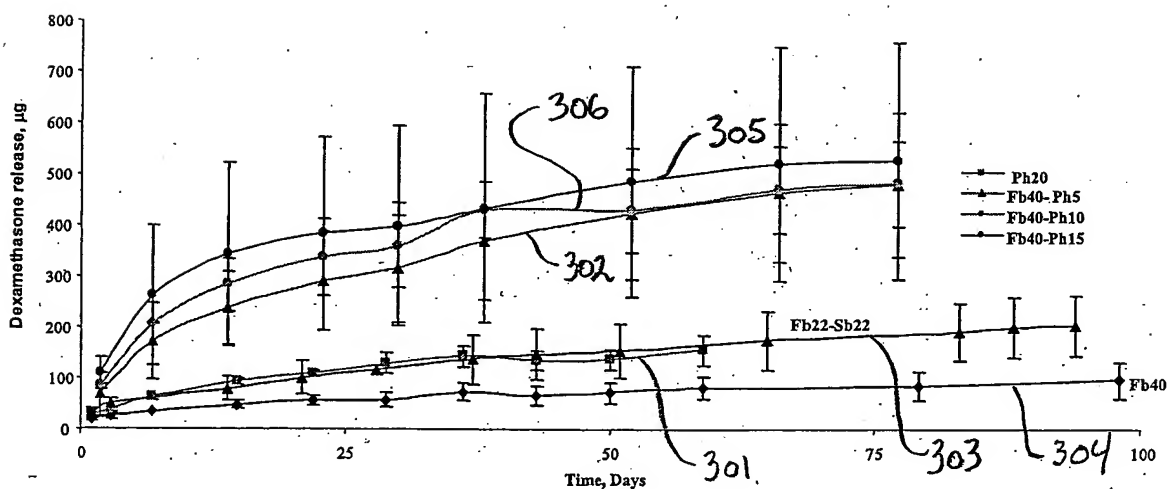


FIG. 17

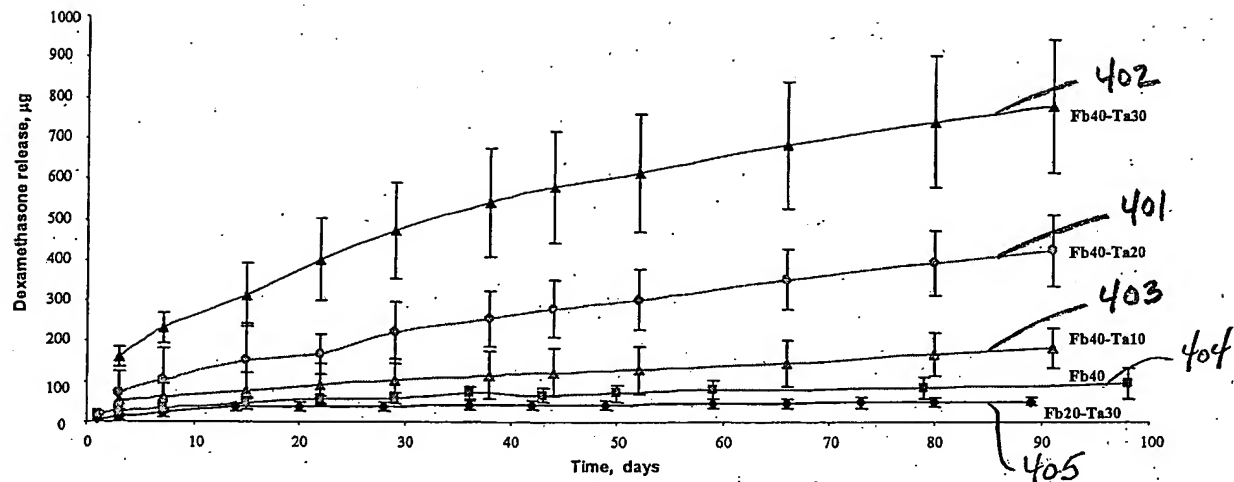


FIG. 18

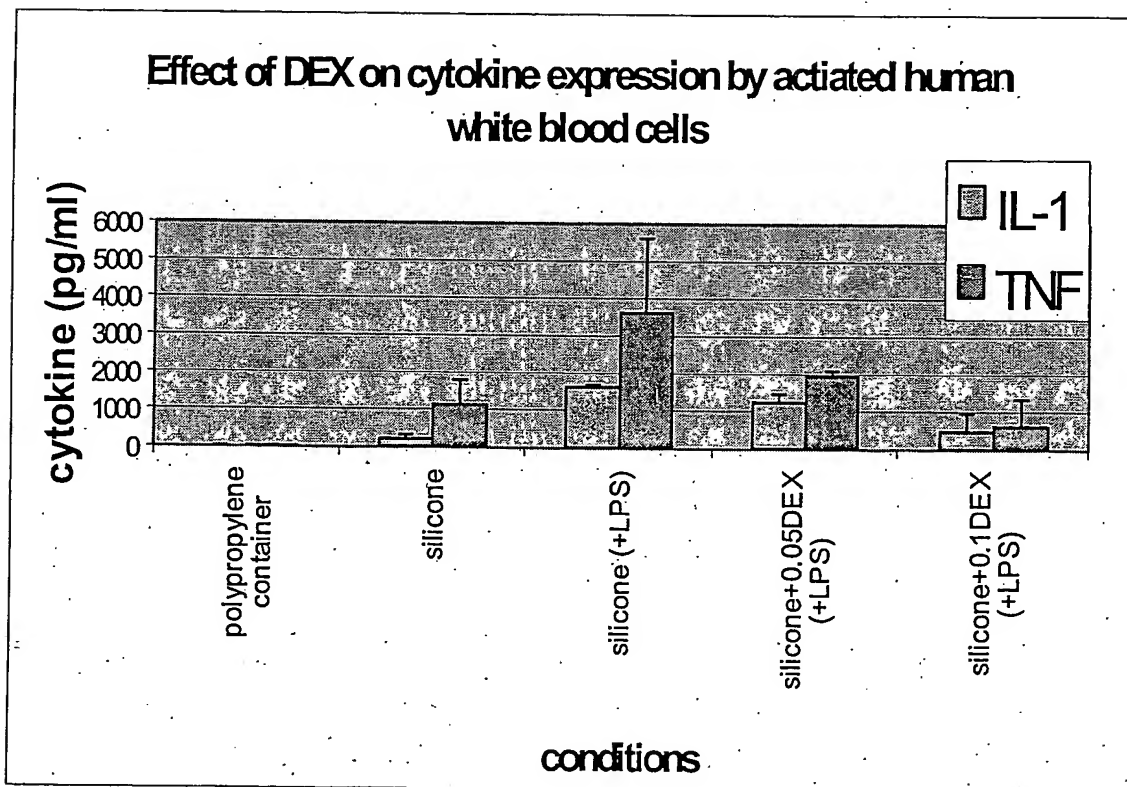




FIG. 19

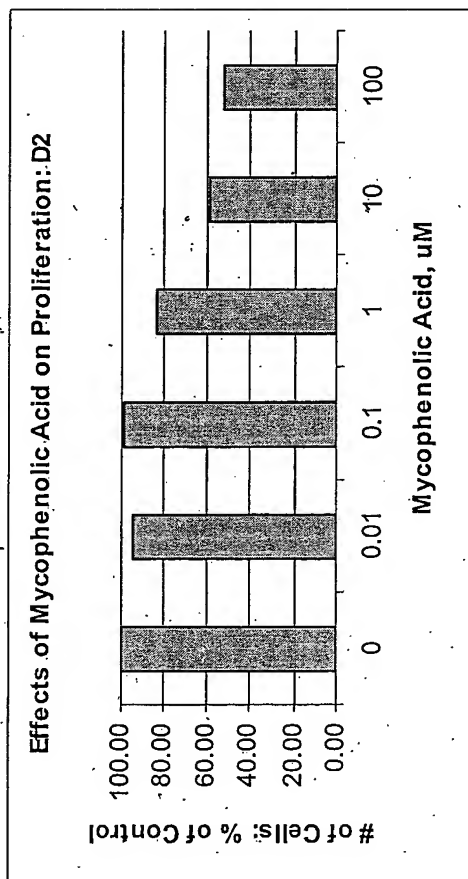


FIG. 21

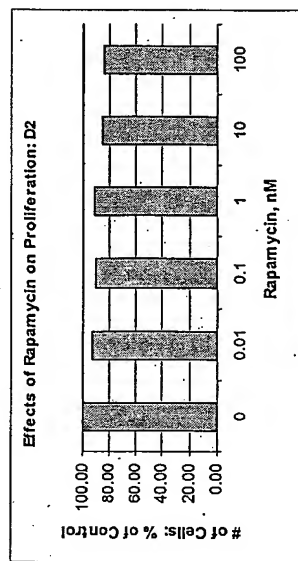


FIG. 20

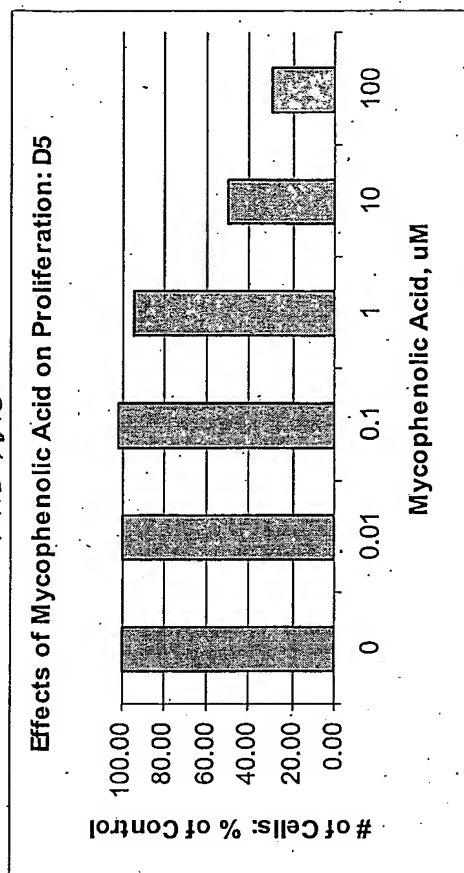


FIG. 22

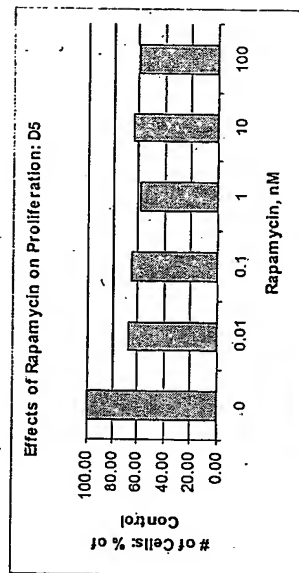


FIG. 28

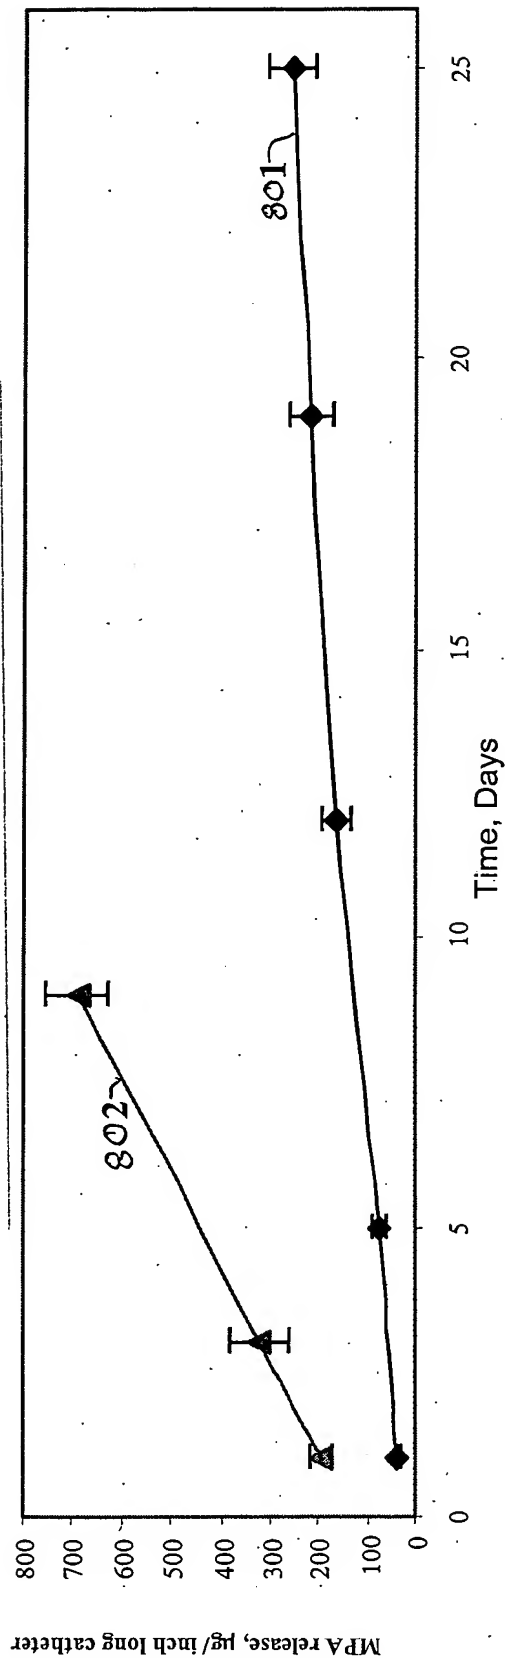


FIG. 24

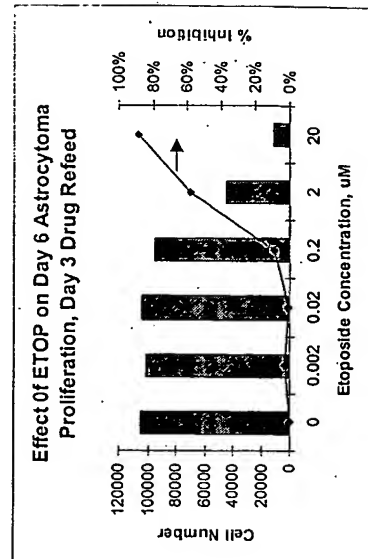


FIG. 23

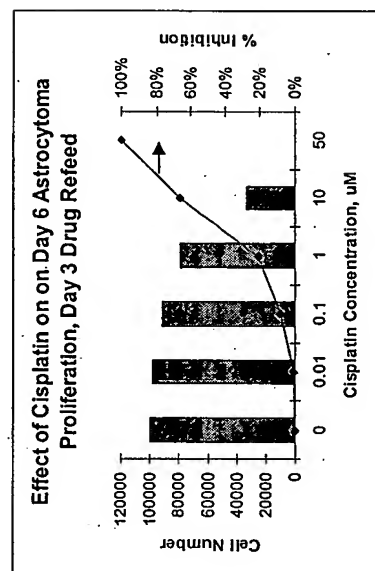


FIG. 25

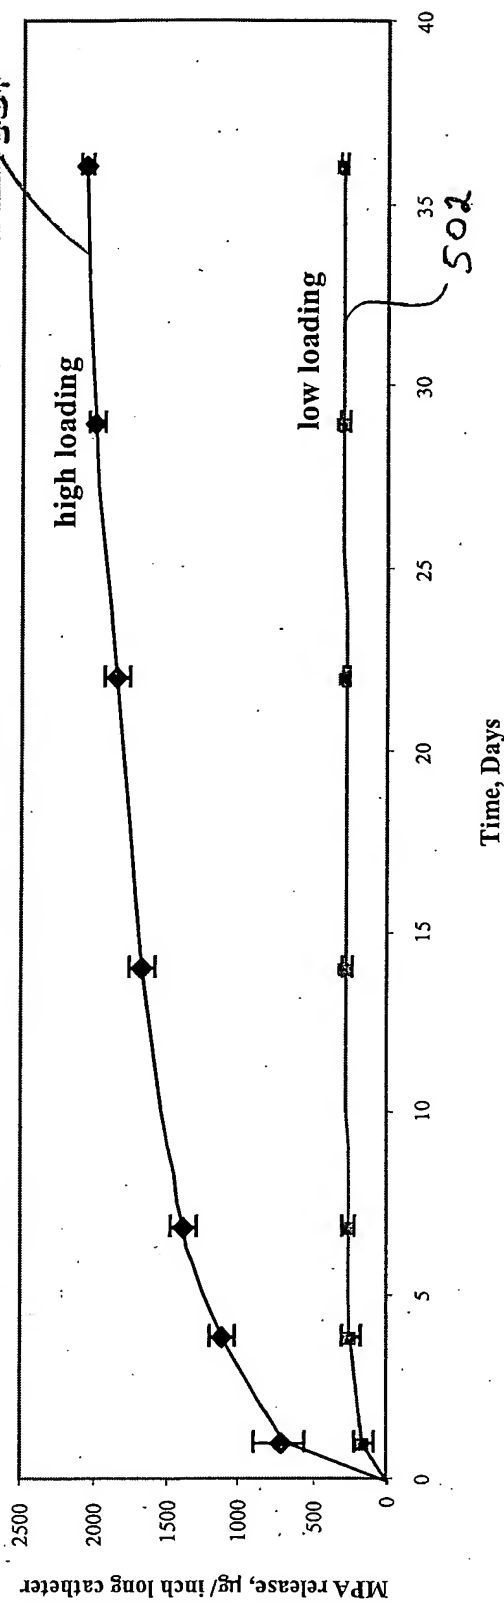


FIG. 26



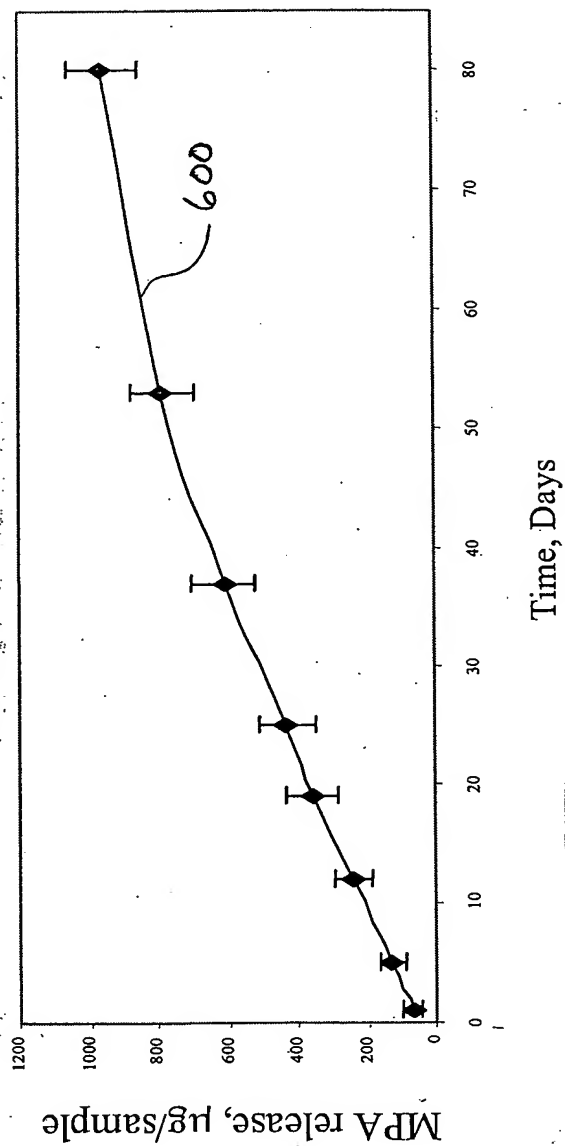


FIG. 27

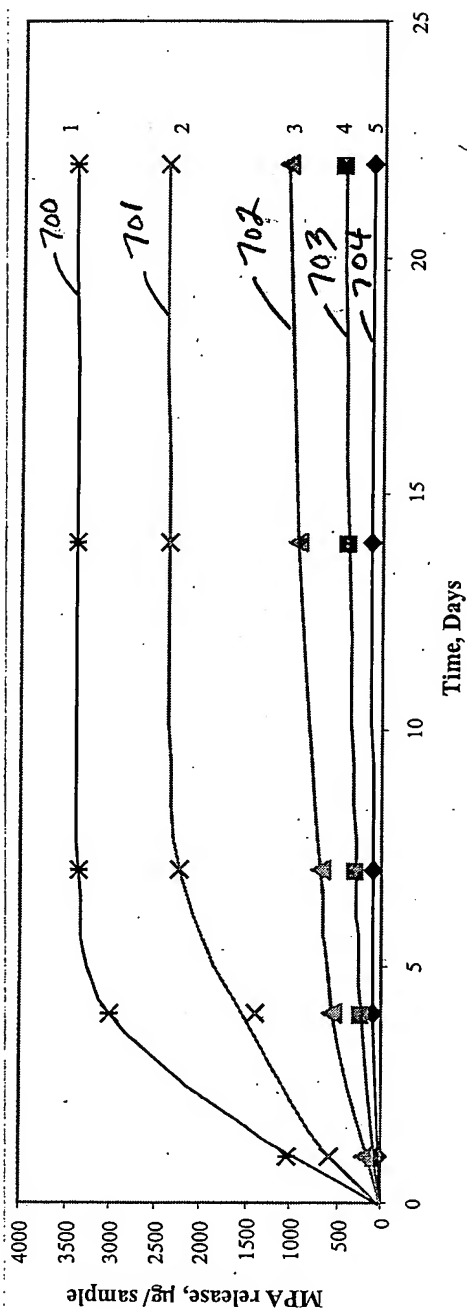

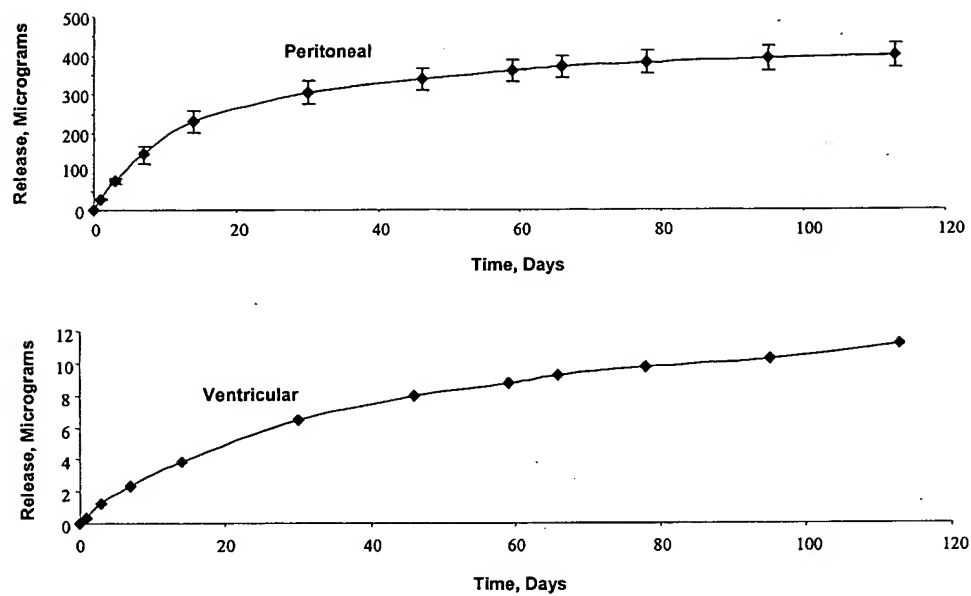

In-vitro release of RAPA from silicone catheters of different sizes.

**Figure 29**